



## Welch Allyn® RetinaVue® 700 Imager


## Welch Allyn® RetinaVue® 700 Imager Battery Charger Assembly Instructions


Mat. No. 728695, 80024084 Ver. C Revision date: 2019-04


Welch Allyn Technical Support: <a href="https://www.welchallyn.com/support">www.welchallyn.com/support</a>

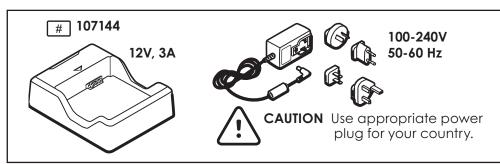




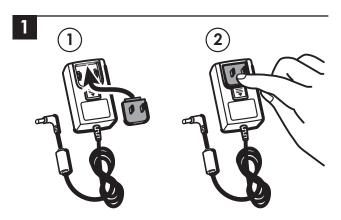

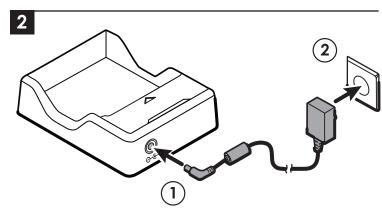

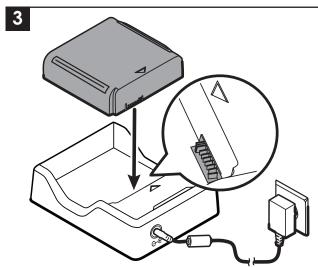

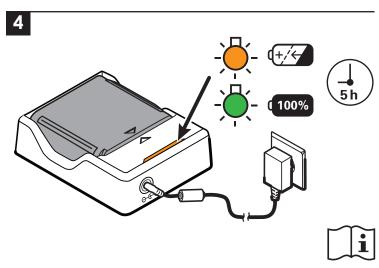



**WARNING** The battery charger (non-medical electrical equipment) shall be situated outside the patient environment (reference IEC 60601-1-1).



**WARNING** Electric shock hazard. Do not open the battery charger or attempt repairs. The battery charger has no user-serviceable internal parts. Inspection and servicing of internal parts shall only be performed by qualified service personnel.



**WARNING** Electric shock hazard. Before cleaning the battery charger, disconnect the AC power cord from the mains outlet and the power source.



**WARNING** Do not use batteries from other sources. This may result in excessive temperatures, fire, or explosion.



 $\textbf{CAUTION} \ \ \textbf{Use appropriate power plug for your country}.$ 



**CAUTION** Do not modify this equipment without authorization of the manufacturer.