



E


1

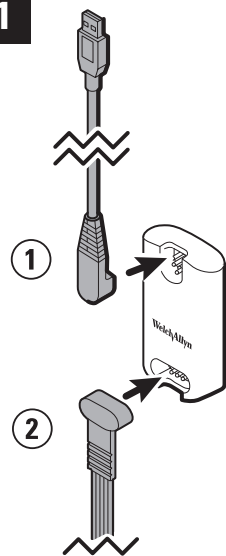


2

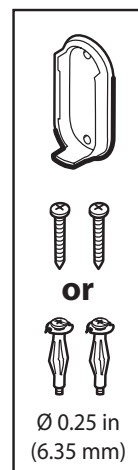


1

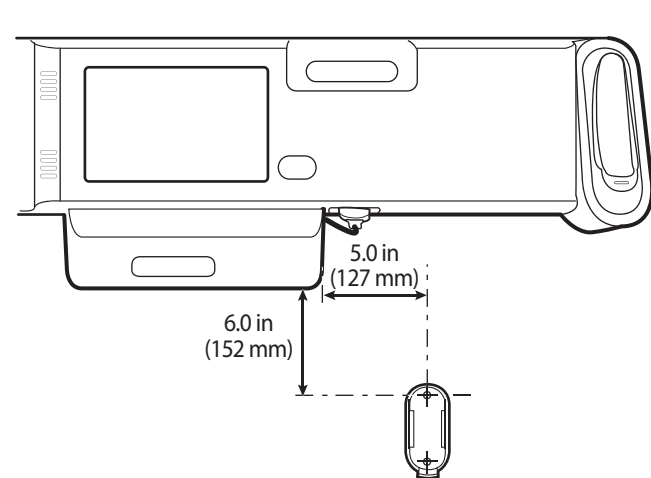


2

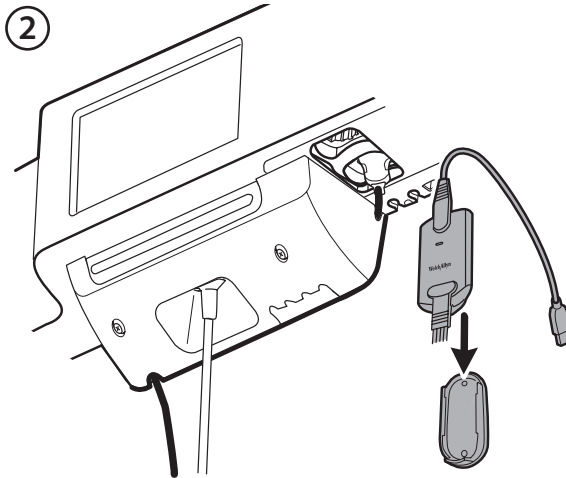


3

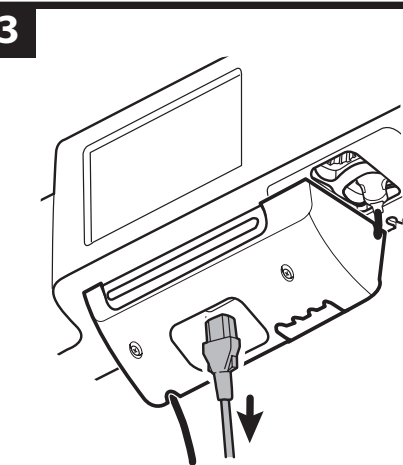


4

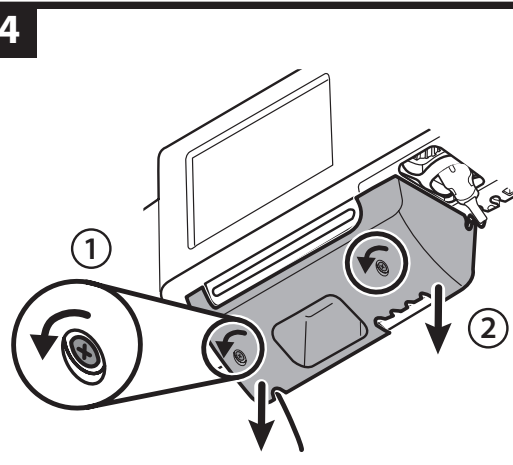


5

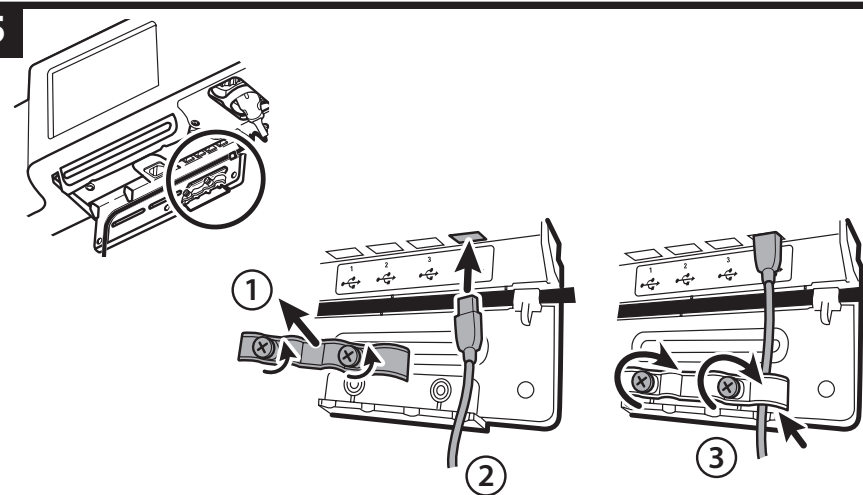

6

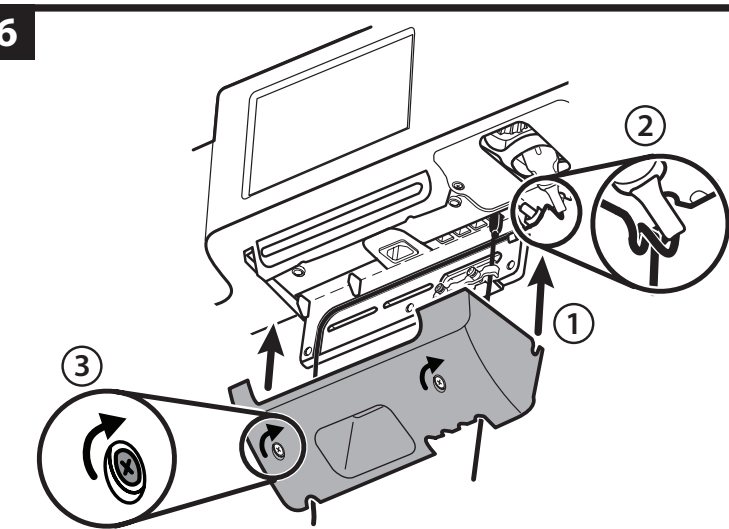



7

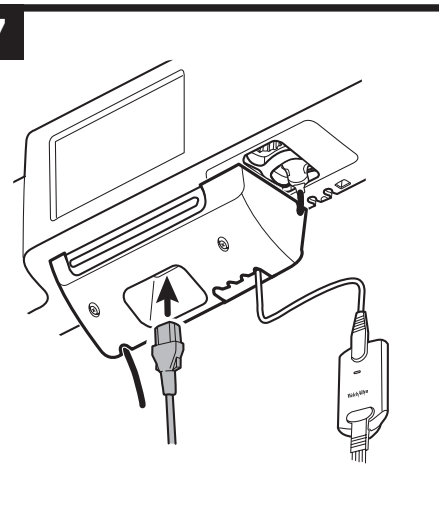


Hillrom™

# Welch Allyn® Connex® Devices ECG Module Assembly Instructions

























Mat. No. 774898, 80029680 Ver. B  
Revision date: 2022-06  
© 2022 Welch Allyn, Inc. All rights reserved.  
Welch Allyn, Inc. is a subsidiary of Hill-Rom Holdings, Inc.

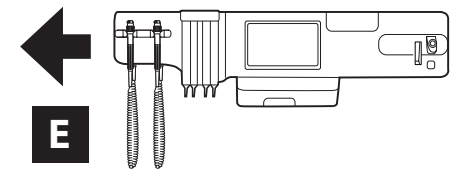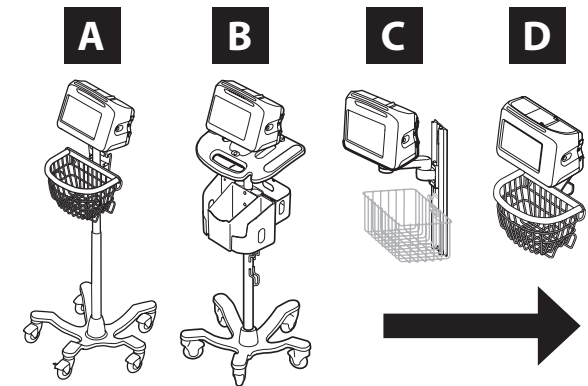






A  
B  
C  
D

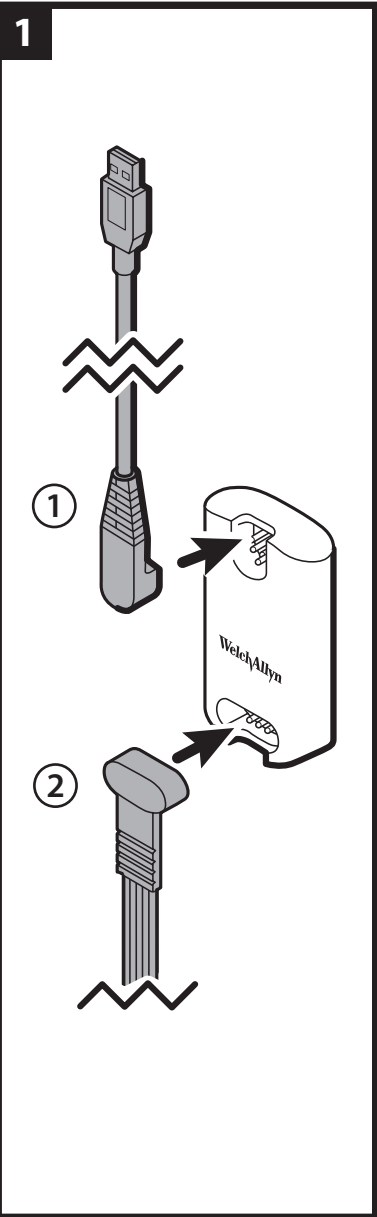

**2**

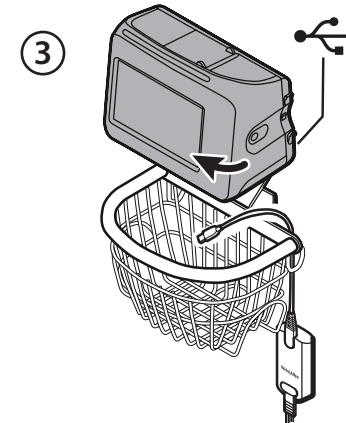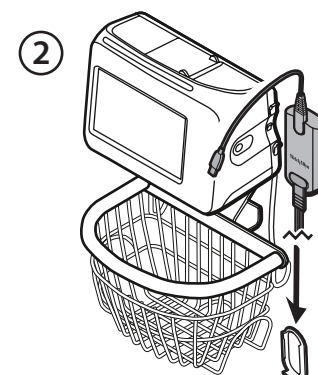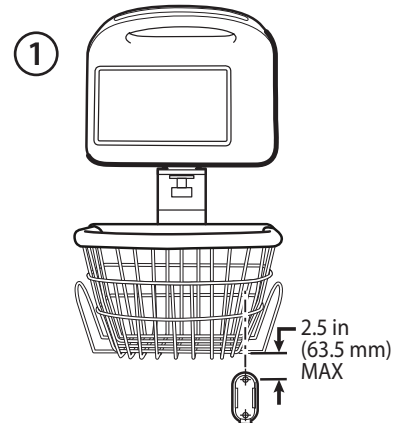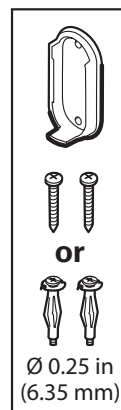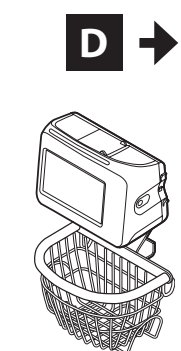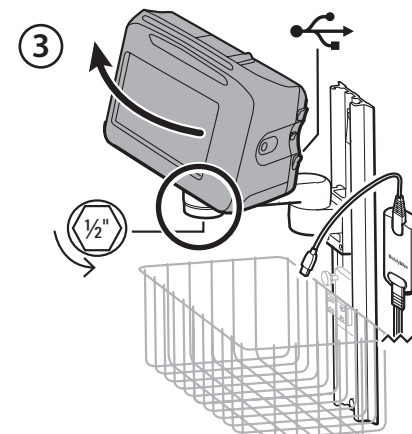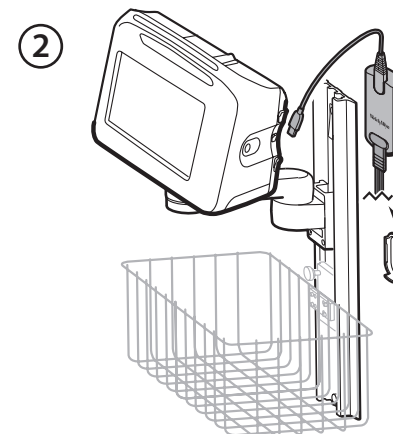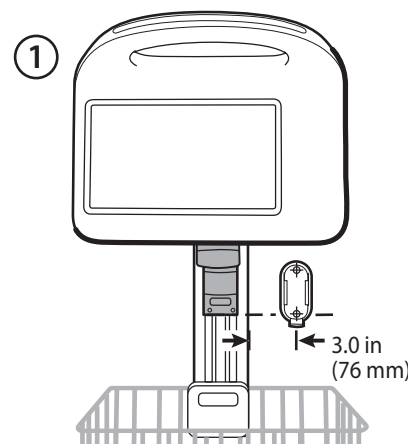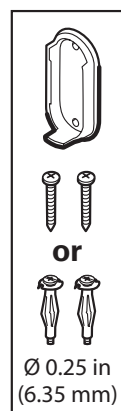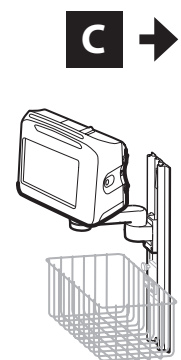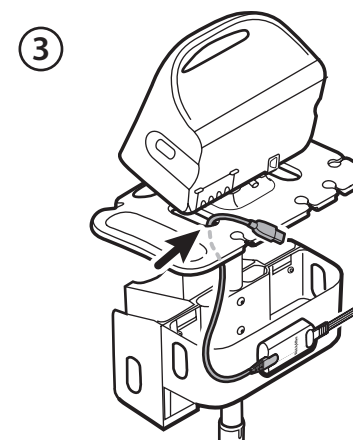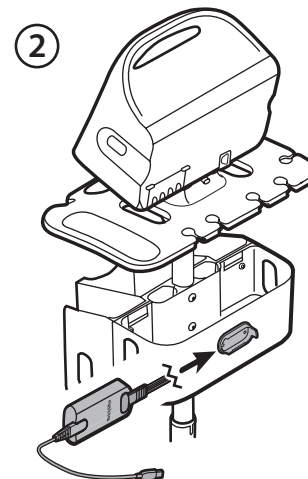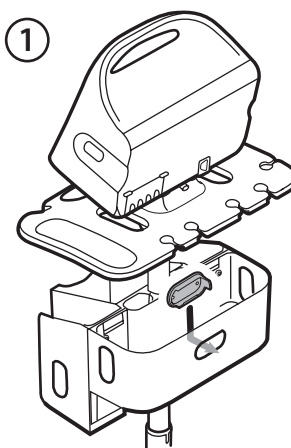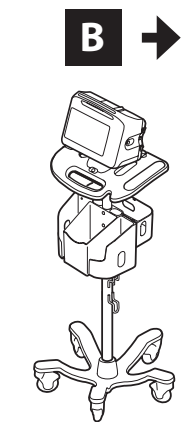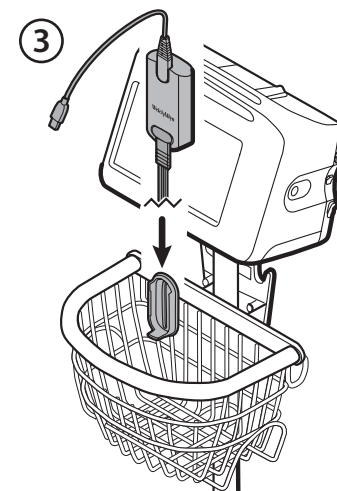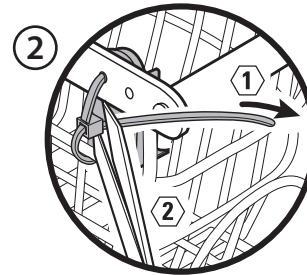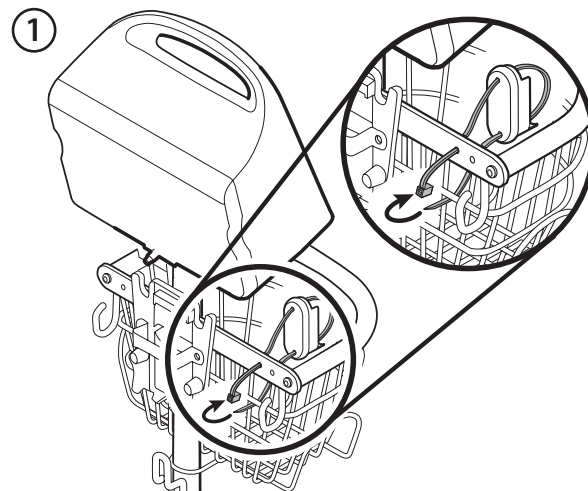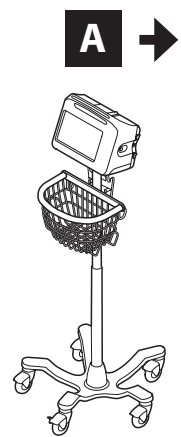

**3**

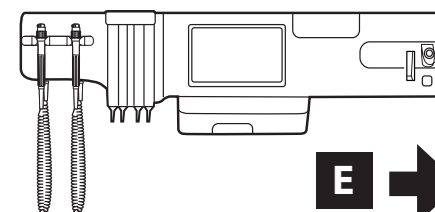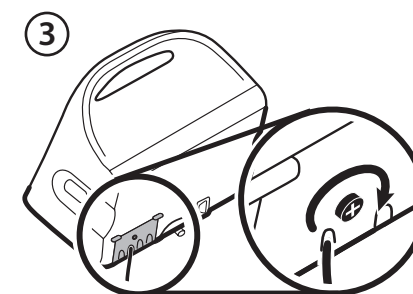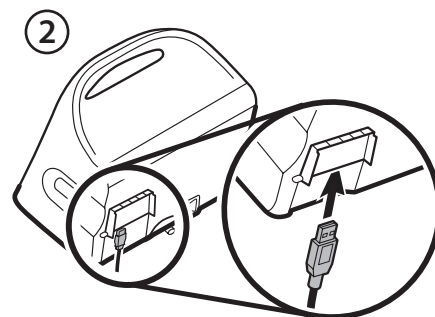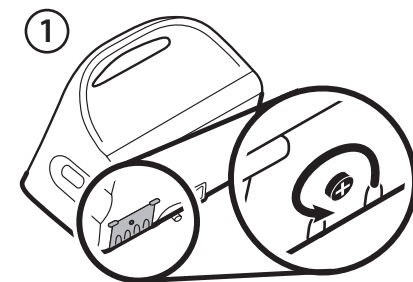

**E** →