



Welch Allyn
Connex 360
Vital Signs Monitor
Startup guide

REF 775743, 80030091 Ver. D
Revision date: 2025-01


Baxter, Welch Allyn and Connex 360 are trademarks of Baxter International Inc. or its subsidiaries.

baxter.com


Baxter Technical Support
baxter.com/contact-us



(91)775743



REF 9000-C360

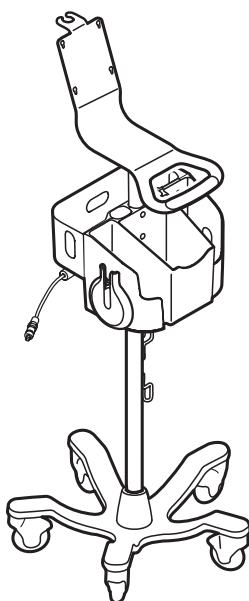

(EN) These instructions are for assembly with 9000-C360 Mobile Stand. Order 9000-GCX for wall mount instructions.


(FR) Ces instructions concernent le montage du support mobile 9000-C360. Commandez le système 9000-GCX pour obtenir les instructions relatives au support mural.

1




①

6mm

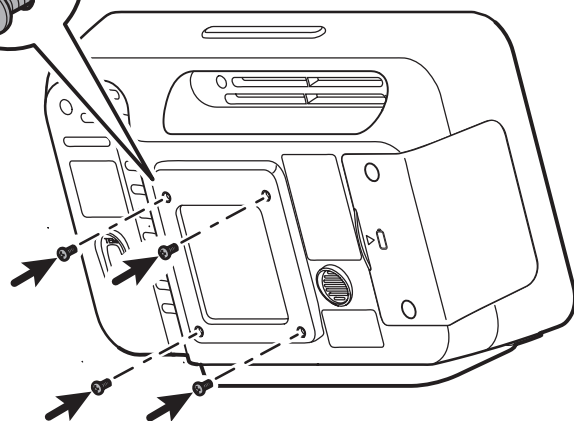


②


7.5+/-0.5 in-lb.
(0.85+/-0.056 Nm)

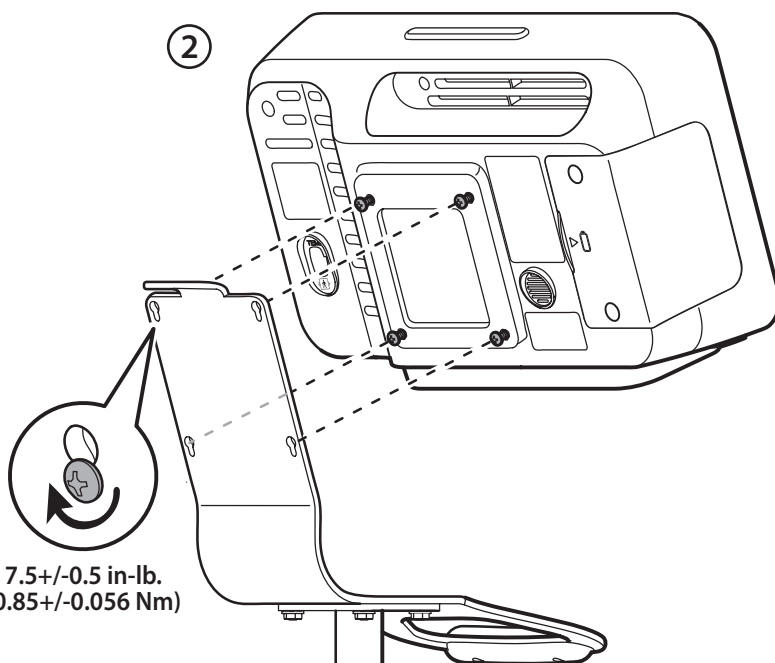


2



1

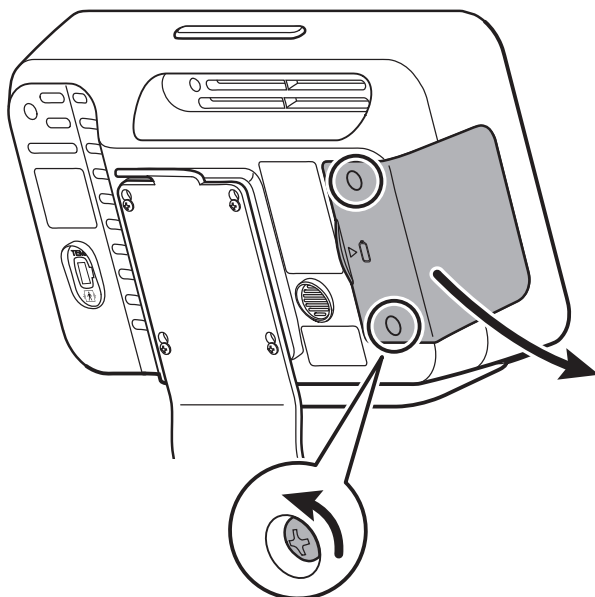


2

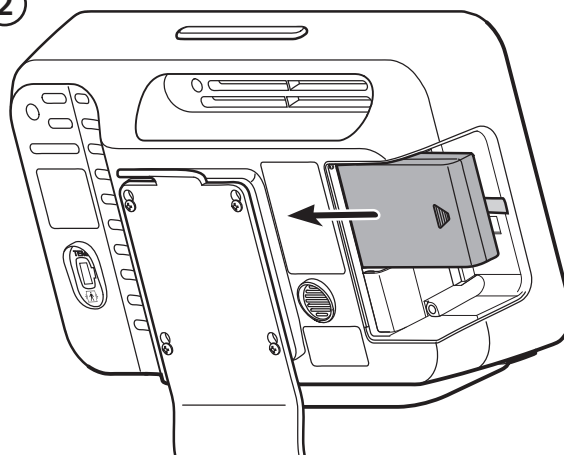


7.5+/-0.5 in-lb.
(0.85+/-0.056 Nm)

3



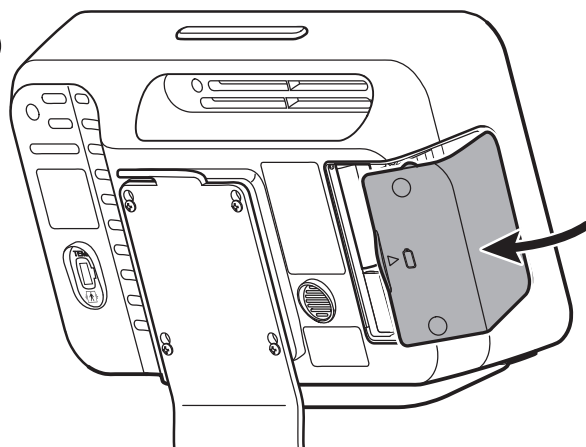


4

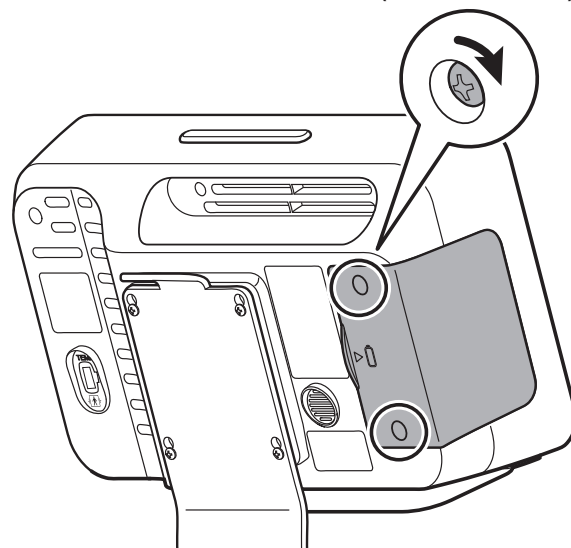



3

NIBP

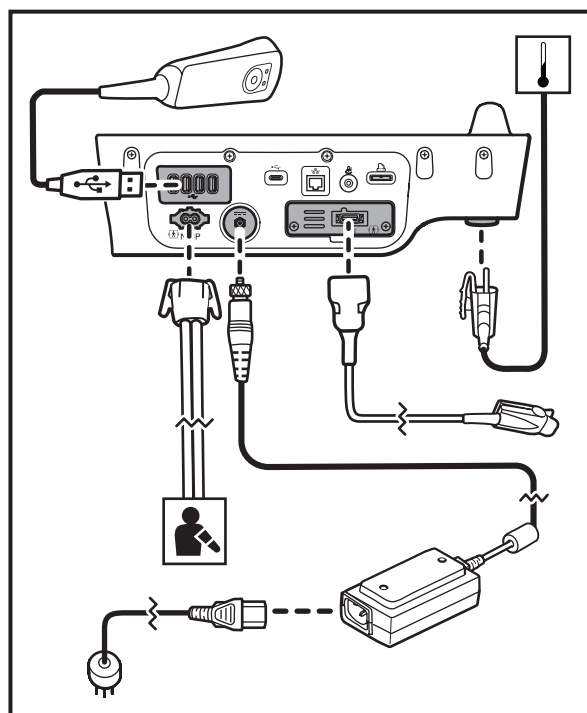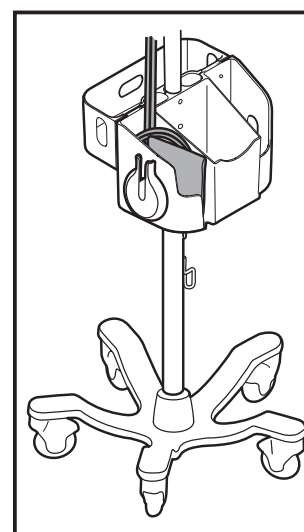
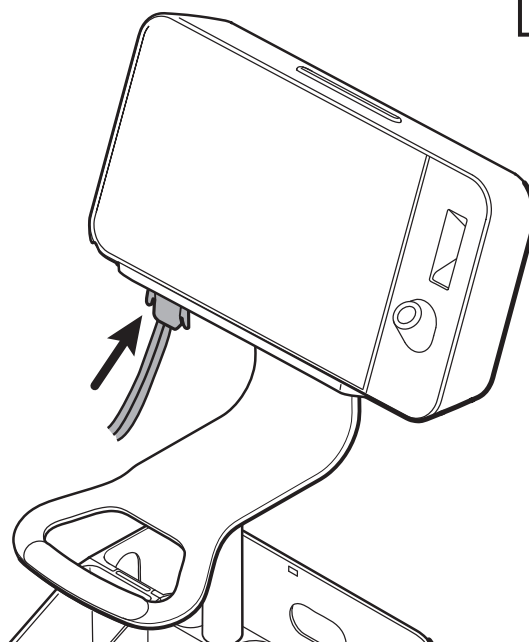


4


SpO2

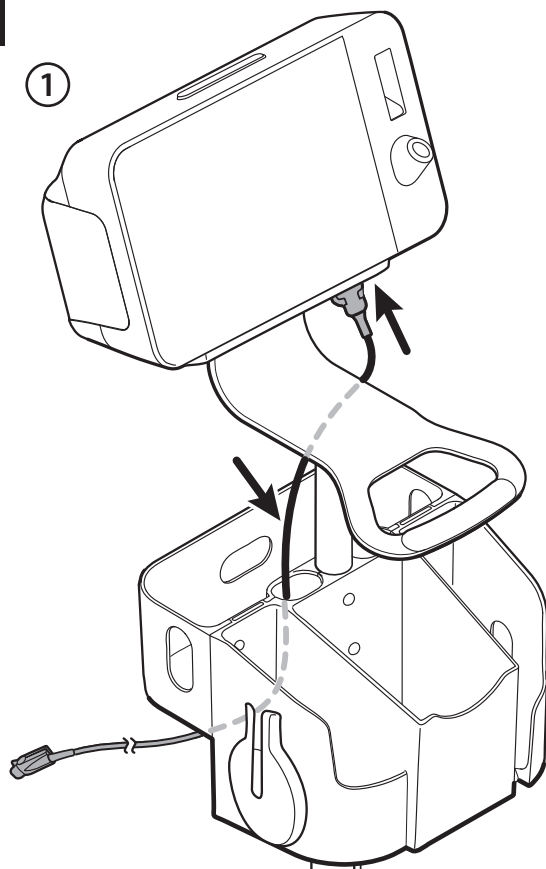


②

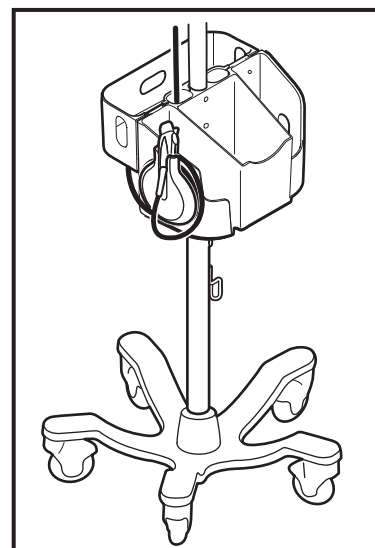


5

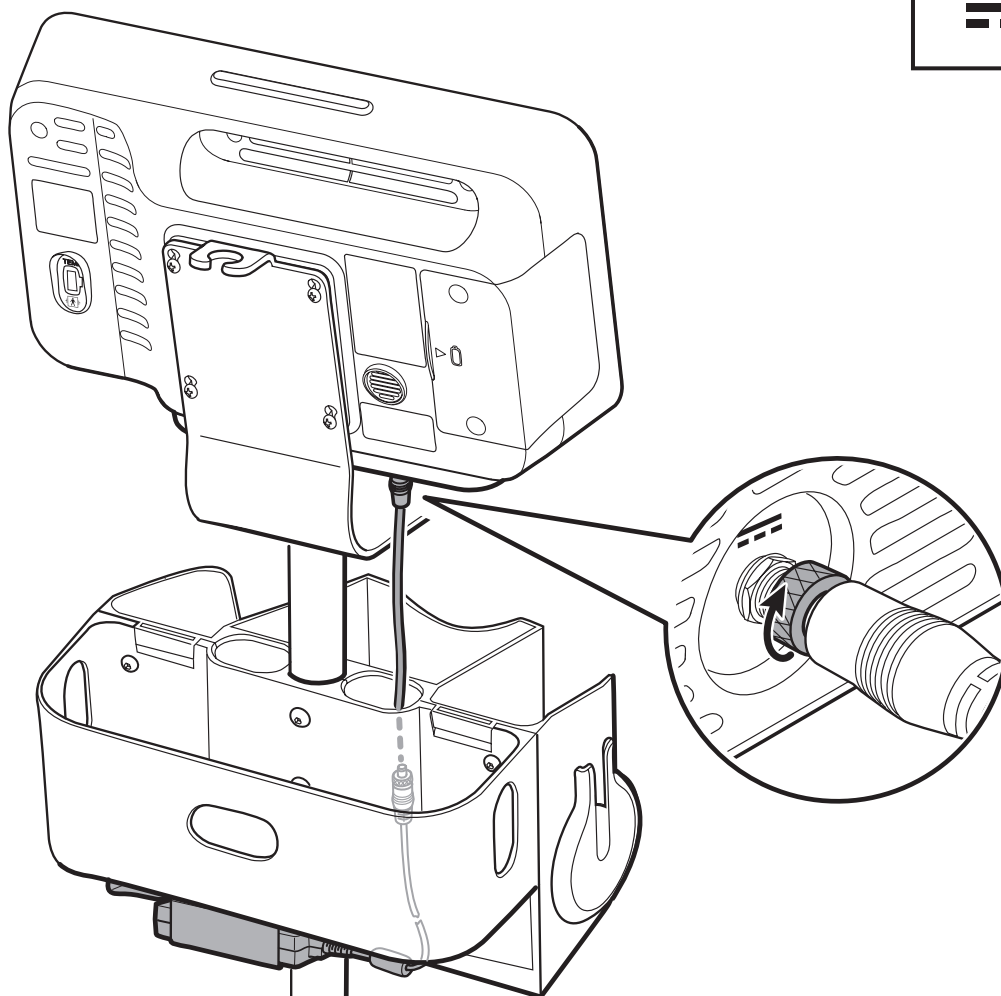

6

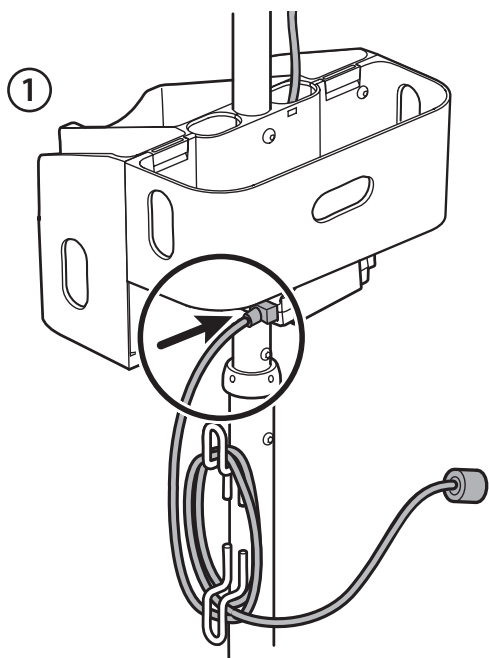



7

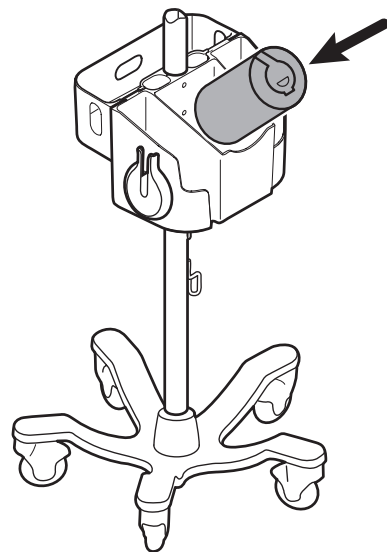


2




Temp



1

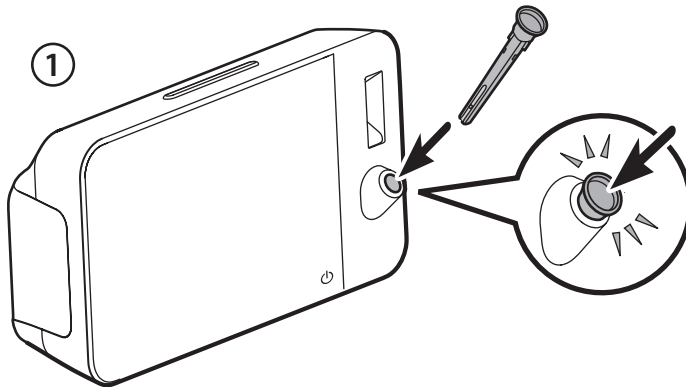

2

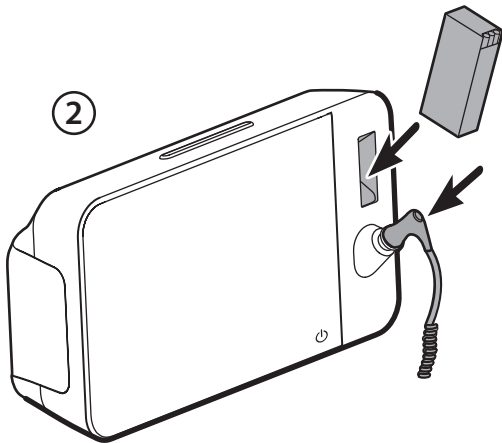

3

